3050 Spruce Street, St. Louis, MO 63103 USA
Tel: (800) 521-8956 (314) 771-5765 Fax: (800) 325-5052 (314) 771-5757
email: techservice@sial.com sigma-aldrich.com


Product Information

Testosterone solution
1.0 mg/mL±2% in 1,2-dimethoxyethane drug standard

Catalog Number **T5411**Lot Number 081M8702
Storage Temperature 2–8 °C

CAS RN 58-22-0

Synonyms: 17β -Hydroxy-3-oxo-4-androstene, 4-Androsten- 17β -ol-3-one, *trans*-Testosterone, 17β -Hydroxy-4-androsten-3-one



Product Description

Molecular Formula: C₁₉H₂₈O₂ Molecular Weight: 288.42

DEA Class: Exempt preparation of Class III

Concentration: 1.00 mg of testosterone/mL of HPLC grade 1,2-dimethoxyethane, concentration verified by UV.

Expiration Date: August 2014

Precautions and Disclaimer


This product is for R&D use only, not for drug, household, or other uses. Please consult the Material Safety Data Sheet for information regarding hazards and safe handling practices.

Storage/Stability

Store the product at $2-8\,^{\circ}$ C. If stored at $2-8\,^{\circ}$ C in an airtight container, protected from light, decomposition of the product is less than 1% in 12 months. After opening, concentration may change due to loss of solvent.


CMW,MAM 07/11-1

70 eV Electron Ionization Mass Spectrum

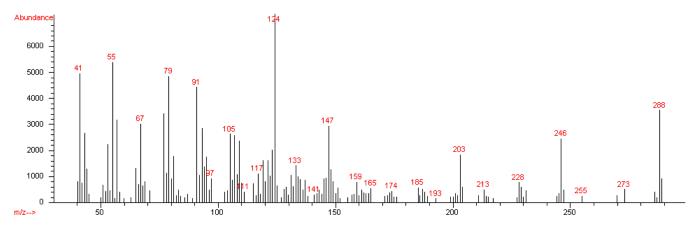

Hewlett-Packard 5890 Series II Gas Chromatograph Hewlett-Packard 5971 Mass Selective Detector Hewlett-Packard G1034C MS ChemStation (HP-DOS series)



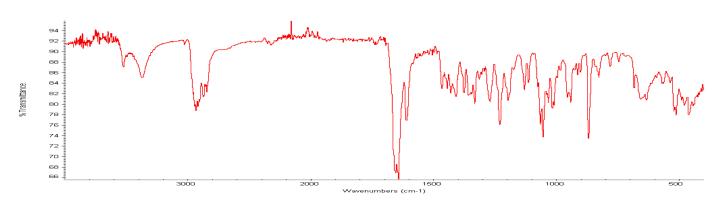


Nicolet 380 FT-IR Thermo Smart Orbit


Ultraviolet Spectrum

Peak 239.5 nm Absorbance 0.6704 Solvent Methanol Dilution 1:99(v/v)

Capillary Gas Chromatography

Column Supelco SPB-1 (Catalog Number 24162)
I.D. 0.20 mm Length 15 m Film Thickness 0.20 μm
Oven Temperature 150 °C (2 minutes), then
15 °C/minute to 300 °C, hold 18 minutes
Injector Temperature 250 °C, Split
Detector Hewlett-Packard 5971
Mass Selective Detector (70 eV, 40-500 m/z)

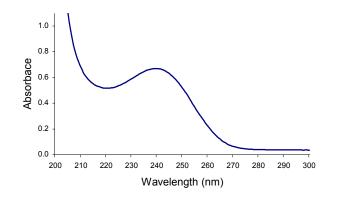

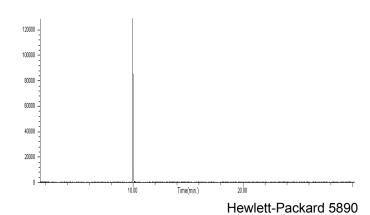

Beckman-Coulter DU 800